TABLE OF CONTENTS
FOR
SERVICE BULLETINS

Bulletin No.	Bulletin Description
D100	Replacement Lamp Shield & Cover Kit to correct: Lamp Shield (Birdcages) falling out of Model L Lighthead After Customer changes bulb or cleans reflector cover.

© Midmark Corporation 2000

Printed in U.S.A.

Return To Table Of Contents

Return To Table Of Contents

Knight® by Midmark

Dental Products Service Bulletin Number: D100

Subject: Lamp Shield (Birdcages) falling out of Model L lighthead after customer changes bulb or cleans reflector cover.

IMPORTANT INFORMATION

This kit pertains to Model L Dental Light.
The new lamp shield contains an embossed alignment designation and the new reflector cover has Unlock / Lock graphic designations.
With the new parts installed the Operator will be able to assure when the lamp shield is in the locked or unlocked position by where the lamp shield designation is aligned to the graphic designations on the cover.

KIT COMPONENTS

Part Number	Description	Qty.
002-0652-00	Kit, Lamp Shield & Cover	1
• 122845	Cover, Stamped Reflector	1
• 152479	Shield, Lamp Assy.	1
• 003-1085-00	Installation Instructions	1

REQUIRED TOOLS

None

REMOVAL / INSTALLATION

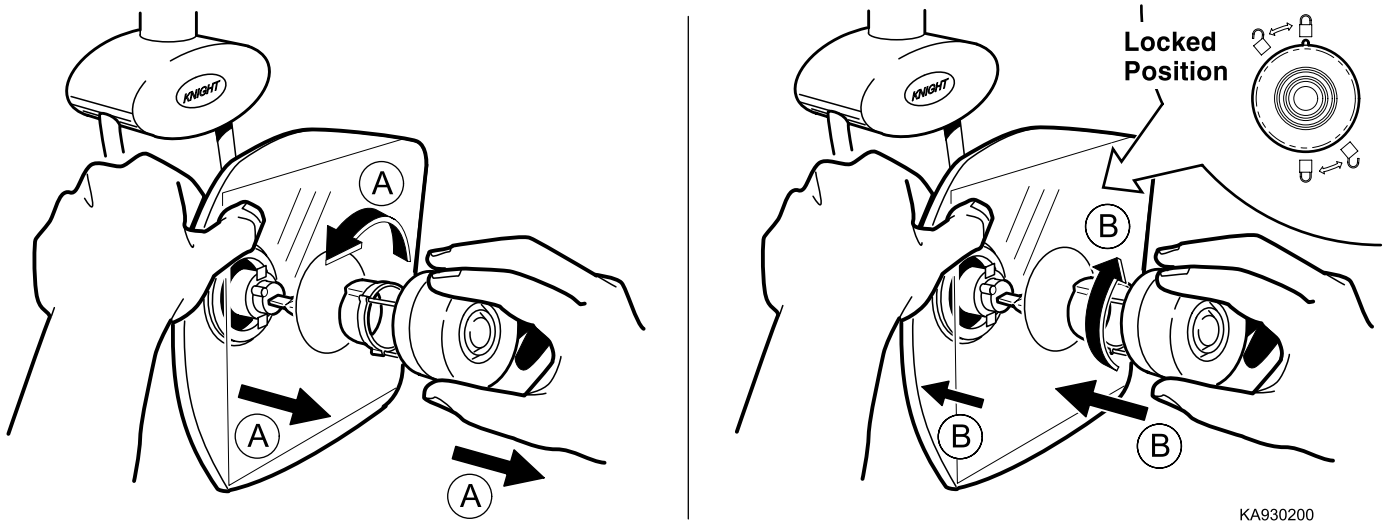

WARNING.

Turn OFF the light and allow lighthead to cool at least 2 minutes before replacement of parts or personal injury could occur.

A. While holding the reflector cover in position, push in and rotate the lamp shield *counter-clockwise* until it stops. Pull outward to remove the lamp shield and reflector cover.

B. Place the new reflector cover in position and insert the lamp shield. While pressing inward, rotate the shield *clock-wise* toward the LOCK graphic until the designator on the reflector is aligned with the graphic.

EQUIPMENT ALERT

Pull outward on the lamp shield to assure it is locked in position.

NOTE

Inform the customer of proper operation in removal and installation procedures of the lamp shield and reflector cover when cleaning the light or changing the bulb.

© Midmark Corporation - 2000

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

Return To Table Of Contents